

□□□□□□□□□□□□ □□□□

1. □□□ microporous □□□□□□□□□□□□□□□□□□□□

2. The □□□□□□□□□□□□□□□□□□□□□□□□□□

□□□□□□□□□□□□□□□□□□□□□□□□□□□□□□□□

□□□ □□□□□

□□□□□□□□□□□□

□□

1. □□□□□□□□□□□□□□□□□□□□

2. CE □□□ ISO □□

3. □□□□

□□□


□□□□□□□□□□□□□□□□□□□□□□□□□□□□□□□□

□□□□□□

□□□□□□□□ 5pcs / bag □ 50pcs / carton □□□

□□□□□□□□□□

□□□□	□□□□□□ □□□□
□□□□	□□□□
□□□	□□□
□□□	□□□□□□□□□□
□□	□
□□□□□□□	5pcs / bag □ 50pcs / carton
□□□□	CE / ISO13485
□□□□	□□□□□□□□□□□□□□□□□□□□□□□□□□□□□□□□
□	□□□□□




orient Honest
MEDICAL INTERNATIONAL





orient Honest
MEDICAL INTERNATIONAL

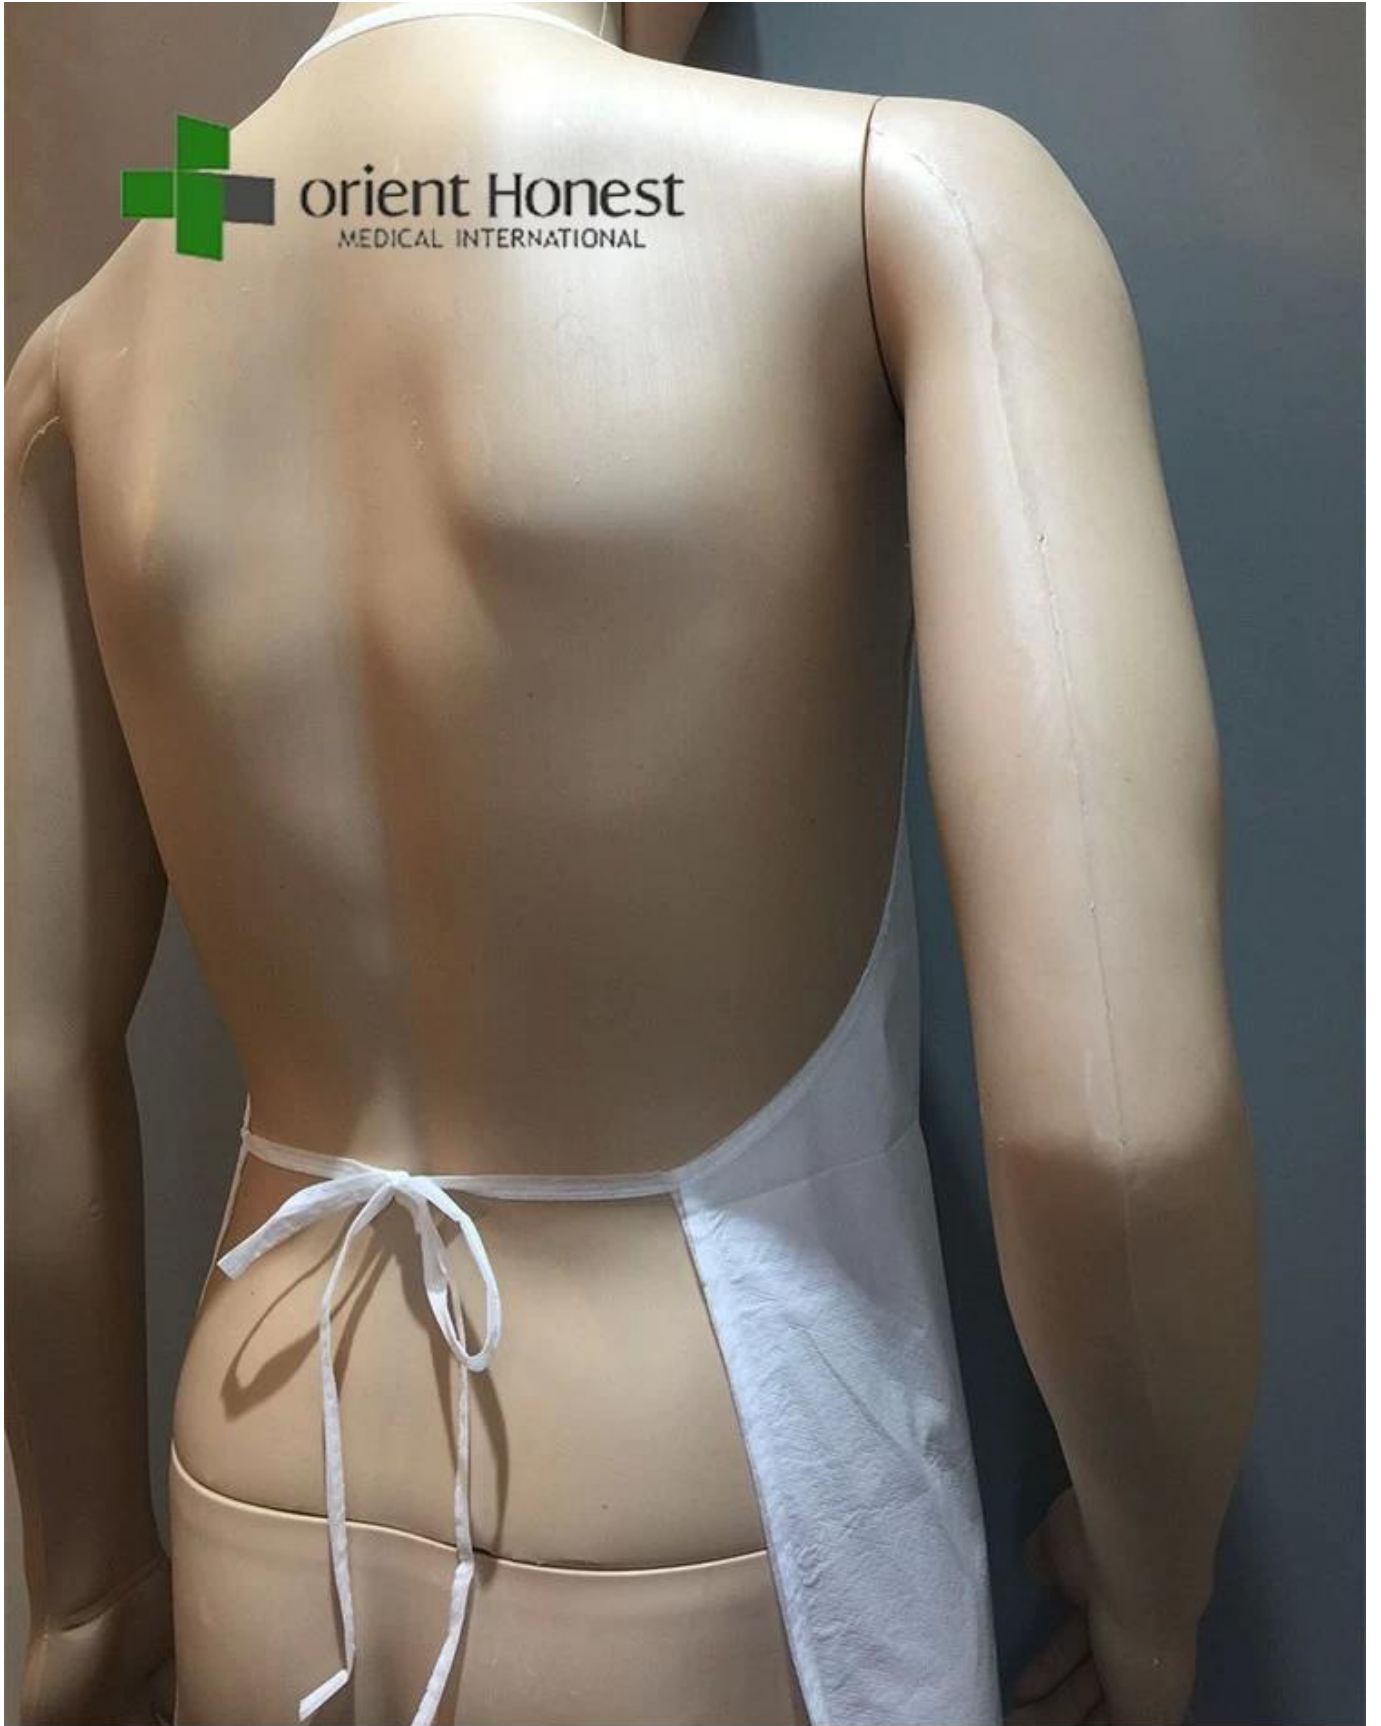



orient Honest
MEDICAL INTERNATIONAL

